


Applies to the following model:

Uno 200 Prod. No. 2010020

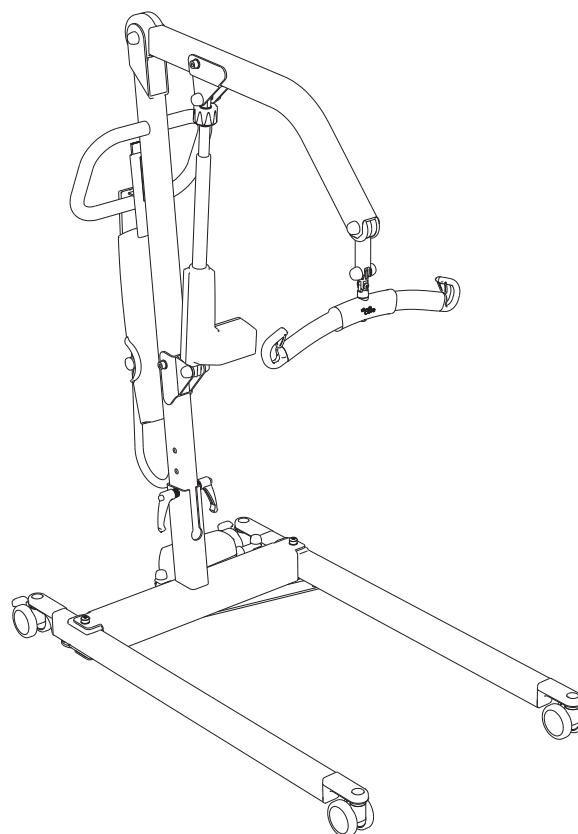

Product Description

Uno 200 is a fully electric mobile lift, i.e., both raising and lowering of the lift arm and width adjustment of the base are done electrically. Uno is designed to be used in most of the common lifting situations, for example transfers between bed and wheelchair, to and from the toilet and bathtub and for lifting to and from the floor.

Uno 200 has three alternative height settings to always enable the optimal lifting height. The intermediate position is the standard setting and is recommended in most cases. The lowest position is appropriate, for example, when lifting from the floor. The highest position is selected when there is a need for extra lifting height; e.g., when lifting to beds and gurneys that are not height-adjustable.

In this document, the person being lifted is referred to as the "patient" and the person helping is referred to as the "caregiver".

△ is a warning triangle used to warn of situations that demand extra care and attention.

Unique for Uno 200 is the variable lifting range and maximum load that is set by a number of adjustments. These adjustments make it possible to optimize Uno for different lifting needs.

In each case, assess the situation to determine how many caregivers are needed to perform a safe and ergonomically correct lifting and transferring operation.

Individual trial fitting and trial use of the sling and other accessories is essential to ensure proper function and safety during the use of the lift.

To ensure maximum safety for caregivers and patients, Uno 200 is equipped for both mechanical and electrical emergency lowering.

IMPORTANT!

Read the instructions for both the patient lift and the lifting accessories before use. Lifting and transferring a patient always involves a degree of risk. A complete understanding of the contents of instructions is essential, and only trained personnel should use the equipment. When in doubt, contact Liko/Hill-Rom.

Table of Contents

Safety Instructions	2
Definitions	3
Technical Data	3
Measurements	4-5
Assembly	6-7
Operation	7-8
Adjustments	9
Charging the Batteries	10
Maximum Load	11
Recommended Lifting Accessories	11-12
Simple Troubleshooting	13
Care and Maintenance	14

△ NOTE! This instruction guide contains information that is important for users of the product. A complete understanding of the contents of the instruction guide is essential, and only personnel who are well informed should use the equipment. Remember to keep the instruction guide readily accessible for users of the product.

Safety Instructions

Before using the lift for the first time, make certain that:

- the lift is assembled according to the assembly instructions
- the lifting equipment is correctly applied to the lift
- the batteries have been charged for at least 12 hours
- you have read and understood the instruction guides for the lift and lifting accessories
- personnel using the lift have received appropriate instructions and training.

Before lifting always make certain that:

- you have selected the correct type, size, material, and design of slings and accessories to safely meet the patient's needs
- lifting accessories are not damaged
- the lifting accessory is correctly applied to the lifting equipment
- the lifting accessory is correctly and securely applied to the patient, so that no personal injury can occur
- the sling's strap loops are correctly fastened to the sling bar hooks when the sling strap is extended, but before the patient is lifted from the underlying surface
- the lift is set for the correct max. load.

△ Unbalanced lifting poses a tipping risk and may damage the lift equipment!

△ Never leave a patient unattended in a lifting situation!



Uno 200 is tested by an accredited testing institute and comply with the requirements of the directives for medical-technical Class 1 products (MDD 93/42/EEC).

Uno 200 complies with the requirements according to IEC 60601-1, IEC 60601-1-2, EN ISO 10535, UL-60601-1 and CAN/CSA C22.2 No. 601.1.


△ No modification of this product is allowed. Contact Liko/Hill-Rom for further information.

Particular care must be taken when using strong sources of electromagnetic interference, such as diathermy, etc, so that cables are not positioned on or near the lift. If you have questions, please consult the responsible assistive-device technician or the supplier.

This equipment is not suitable for use in the presence of flammable mixtures.

Maximum load: 160 kg (350 lbs) / 200 kg (440 lbs) depending on mounting alternative (see page 5).

Definitions

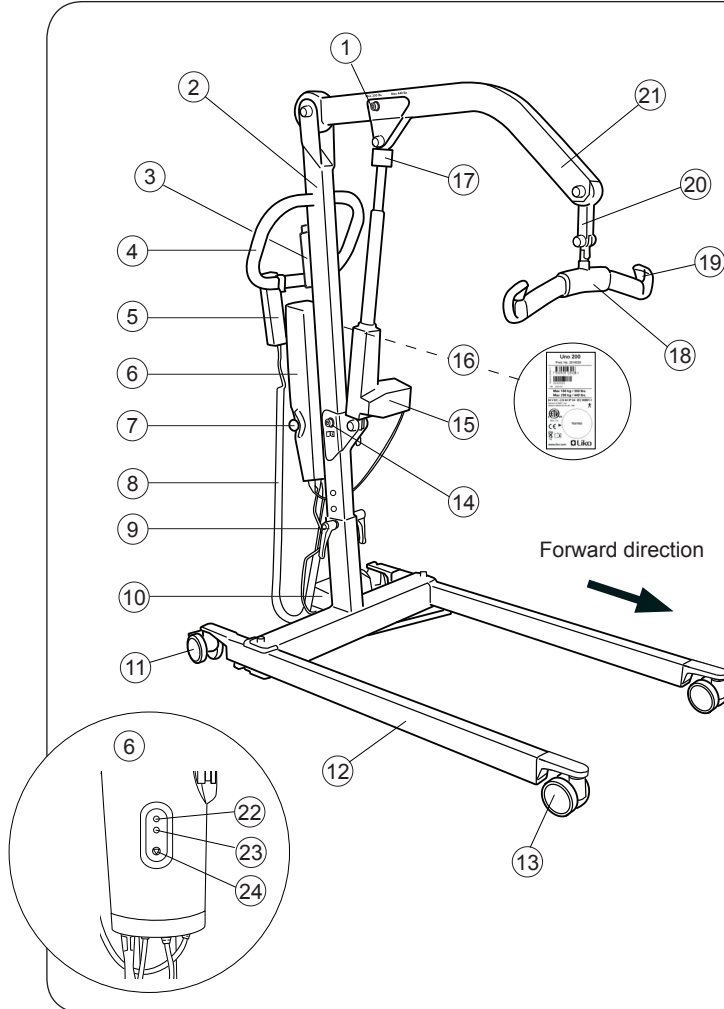

1. Upper attachment (lift motor)
2. Lift mast
3. Holder for quick reference guide with colour codes for sling sizes
4. Manoeuvring handle
5. Hand control
6. Control unit with built-in battery
7. Emergency stop
8. Cable for hand control
9. Locking handle
10. Motor for base-width adjustment
11. Rear wheels with brake
12. Base
13. Front wheels
14. Lower attachment (lift motor)
15. Lift motor (incl. actuator)
16. Product decal
17. Emergency lowering (mechanical)
18. Sling bar
19. Safety latches
20. Flexlink
21. Lift arm
22. LED (yellow light) - charger connected
23. LED (green light) - lift activated
24. Emergency lowering (electrical)

Technical Data

Max. load:	160 kg (350 lbs)/200 kg (440 lbs) depending on mounting alternative
Material:	Painted steel with lacquer top coat.
Weight:	Total: 40 kg (88 lbs) Heaviest dismountable part: 20.5 kg (45 lbs)
Wheels:	Front: 75 mm (2.9 in) twin wheels. Rear: 75 mm (2.9 in) lockable twin wheels.
Turning diameter:	1330 mm (52.4 pulg.)
Emergency lowering:	Mechanical and electrical
Lifting speed (without load):	22 mm (0.9 in)/s for max. load 160 kg (350 lbs) 18 mm (0.7 in)/s for max. load 200 kg (440 lbs)
Sound level:	42 dB(A)
Protection class:	IP X4
Expected life time:	10 years

Operating forces of controls:	Buttons on hand control: 4 N Buttons on display: 4 N
Electrical data:	24 V
Intermittent operation:	Int. Op 10/90, active operation max 2 min. Out of a time of 100, active must be less than 10, though not more than 2 min
Batteries:	2 pcs. 12 V, 2,9 Ah, valve-regulated lead-acid gel-type batteries. New batteries are provided by your Liko representative.
Battery charger:	External charger, 100-240 V AC, 50-60 Hz, max 500 mA.
Lift motor:	24 V, permanent magnet motor with mechanical safety mechanism
Motor for base:	24 V, permanent magnet motor



The device is intended for indoor use.




Type B degree of protection against electrical shock.




Class II equipment.

Measurements


Side view

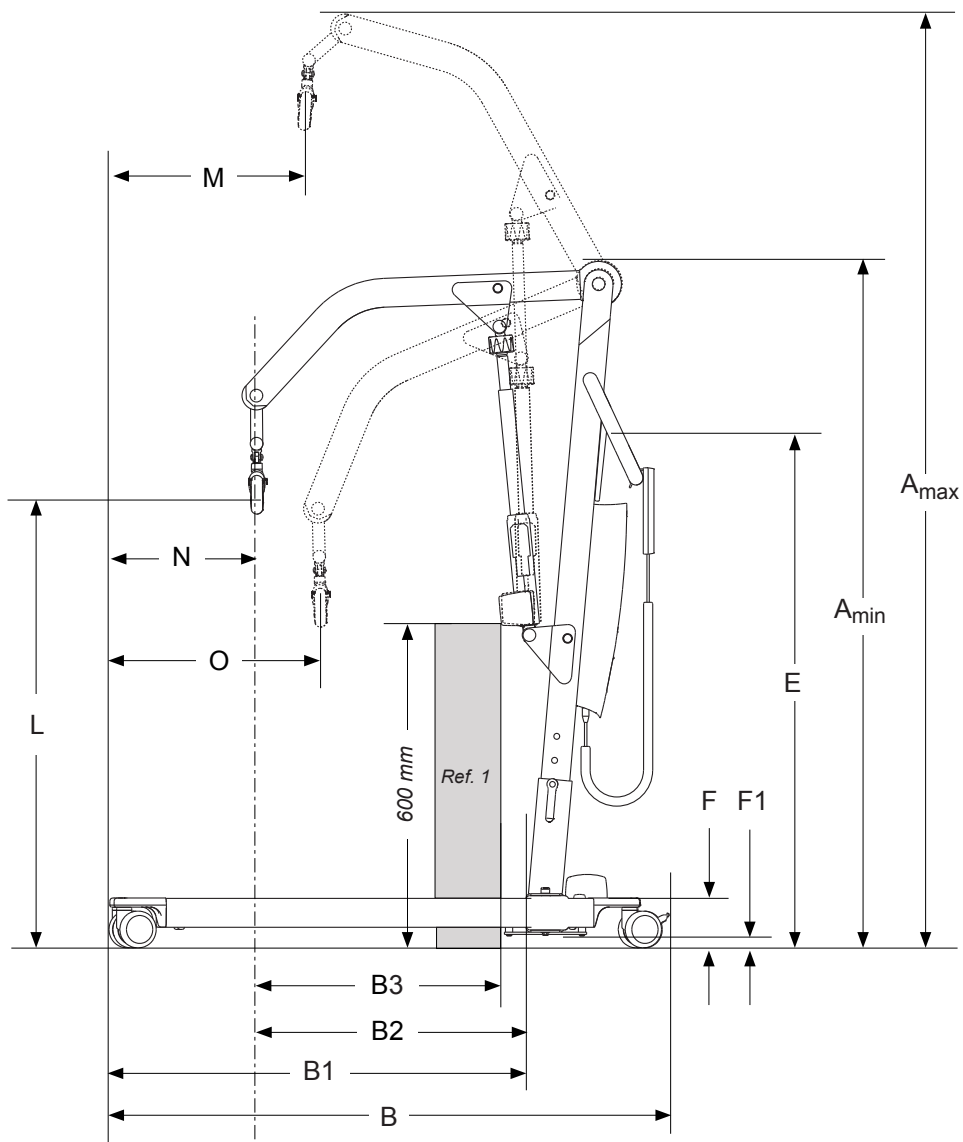

Top view

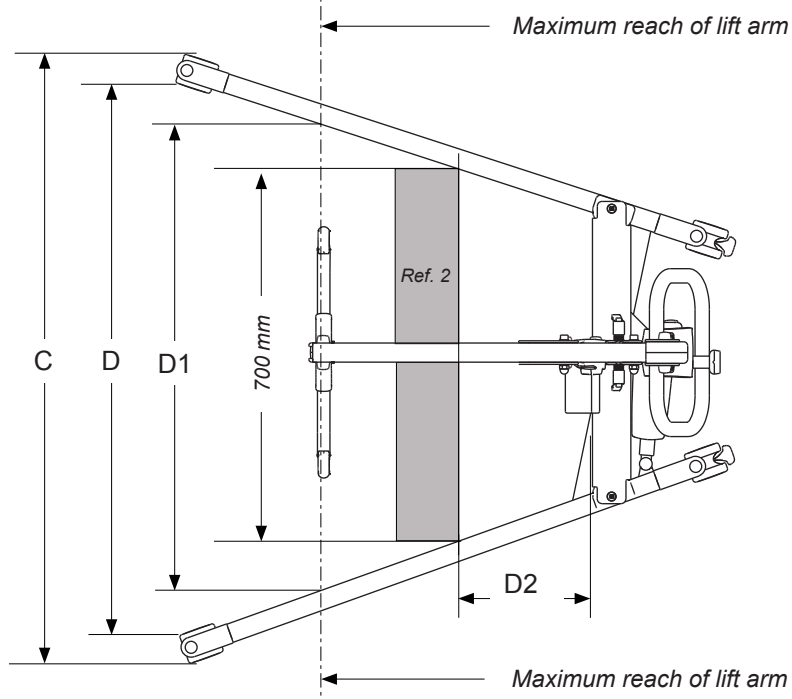

Adjustments of maximum load/lifting height

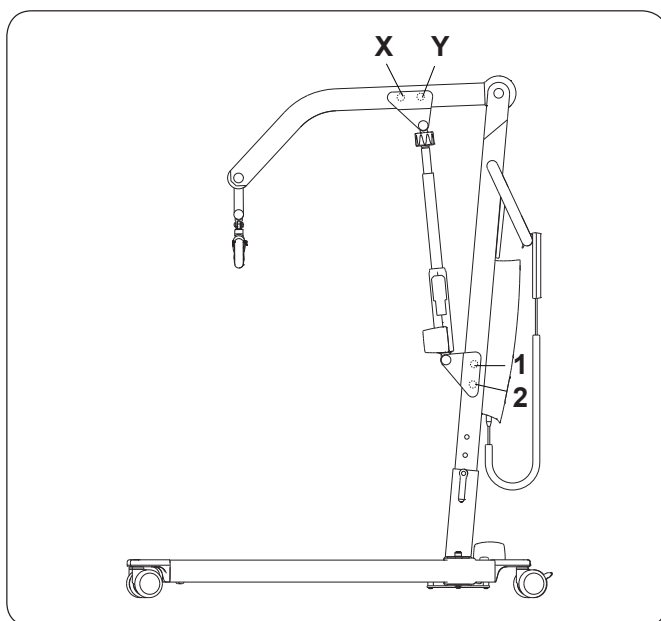

The lift motor can be mounted in four different combinations:

- X1: outer position (X) on the lift arm
upper position (1) on the lift mast
- X2: outer position (X) on the lift arm
lower position (2) on the lift mast
- Y1: inner position (Y) on the lift arm
upper position (1) on the lift mast
- Y2: inner position (Y) on the lift arm
lower position (2) on the lift mast

The different mounting alternatives affect the lift's lifting height and maximum allowable load. See "Table of measurements" below.

Table of measurements

Max. load in kg. Dimensions in mm.

Mounting alternative	Max. load	A*		B	B1	B2	B3**	C		D		D1	D2**	E*	F	F1	L*		Lifting range	M	N	O
		max	min					max	min	max	min						max	min				
X1	200	1835 1785 1735	1430 1380 1330	1220	910	620	620 600 545	1110	675	1000	570	875	255	1080 1030 980	105	20	1590 1540 1490	710 660 610	885	370	295	425
X2	200	1755 1705 1655	1430 1380 1330	1220	910	620	605 545 545	1110	675	1000	570	875	255	1080 1030 980	105	20	1495 1445 1395	630 580 530	870	340	295	495
Y1	160	1940 1890 1840	1430 1380 1330	1220	910	620	615 595 540	1110	675	1000	570	875	255	1080 1030 980	105	20	1705 1655 1605	675 625 575	1035	440	295	460
Y2	160	1845 1795 1745	1430 1380 1330	1220	910	620	605 545 545	1110	675	1000	570	875	255	1080 1030 980	105	20	1600 1550 1500	565 515 465	1040	370	295	570

Max. load in lbs. Dimensions in inch.

Mounting alternative	Max. load	A*		B	B1	B2	B3**	C		D		D1	D2**	E*	F	F1	L*		Lifting range	M	N	O
		max	min					max	min	max	min						max	min				
X1	440	72.2 70.3 68.3	56.3 54.3 52.3	48	35.8	24.4	24.4 23.6 21.4	43.7	26.5	39.3	22.4	34.4	10	42.5 40.5 38.5	4.1	0.8	62.6 60.6 58.6	28 26 24	34.6	14.5	11.6	16.7
X2	440	69.1 67.1 65.2	56.3 54.3 52.3	48	35.8	24.4	23.8 21.4 21.4	43.7	26.5	39.3	22.4	34.4	10	42.5 40.5 38.5	4.1	0.8	58.8 56.8 54.8	24.8 22.8 20.8	34	13.4	11.6	19.4
Y1	352	76.4 74.4 72.4	56.3 54.3 52.3	48	35.8	24.4	24.2 23.4 21.3	43.7	26.5	39.3	22.4	34.4	10	42.5 40.5 38.5	4.1	0.8	67.1 65.1 63.1	26.6 24.6 22.6	40.5	17.3	11.6	18.1
Y2	352	76.4 74.4 72.4	56.3 54.3 52.3	48	35.8	24.4	23.8 21.4 21.4	43.7	26.5	39.3	22.4	34.4	10	42.5 40.5 38.5	4.1	0.8	63 61 59	22.3 20.3 18.3	40.7	14.5	11.6	22.4


* Measures vary depending on height setting level, see "Assembly" page 6. NOTE! The measures apply for a lift equipped with standard sling bar and standard wheels. Before changing lifting equipment or wheels, ensure that the lift still achieves the desired lifting height.

** Reference measurements according to Standard EN ISO10535:2006.


Assembly

Before assembling, make sure you have the following components:


- Lift mast with: lift arm, lift motor (incl. actuator), holder for quick reference guide, control unit and sling bar with safety latches
- Base with motor for base-width adjustment
- Hand control, incl. cable
- Locking handles (1 pair)
- Instruction guide and quick reference guide
- Tools: 8 mm Allen wrench 17 mm closed-end wrench
- Battery charger
- Cable cover incl. screws (2 pcs).

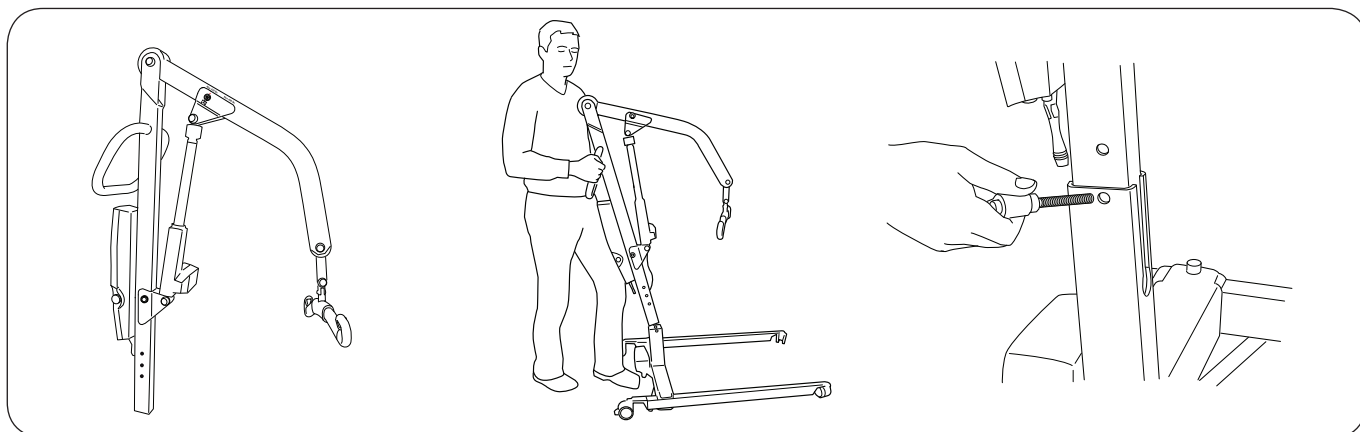


1. On delivery, the lift is set for a max. load of 160 kg.
2. Lock both rear wheels. Place the lift mast in the tube on the base.
3. The lifting height can be set at three different levels. The distance between two holes is 50 mm (2 in). The middle hole is recommended in most cases. See page 9 for more detailed information on the adjustment options.

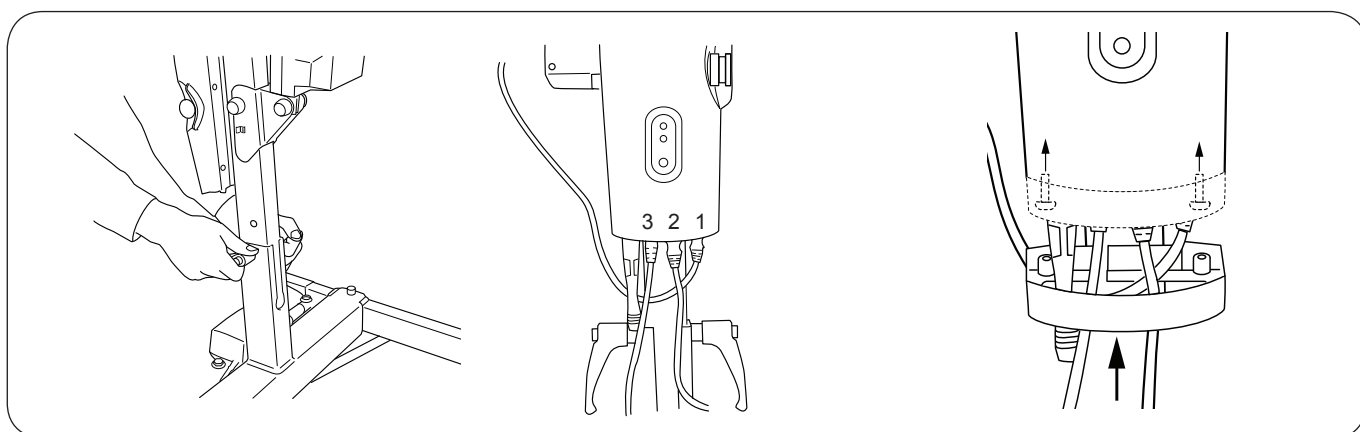


4. Secure the lift mast by using the accompanying locking handles. Adjust the position of the handles so that they point downward.
5. Connect cables as follows:
 - Lift motor cable to socket 1
 - Base-motor cable to socket 2
 - Hand control to socket 3.
6. Guide the cables through the opening on the cable cover. Press the cable cover up into position. Use a screwdriver to secure the cable cover with the accompanying screws (2 pcs).

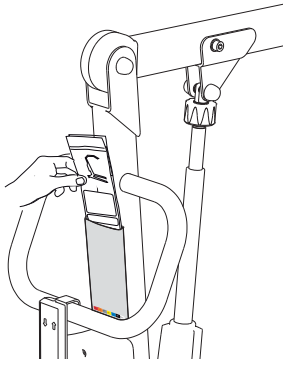

7. Place the quick reference guide in its intended holder on the lift mast.

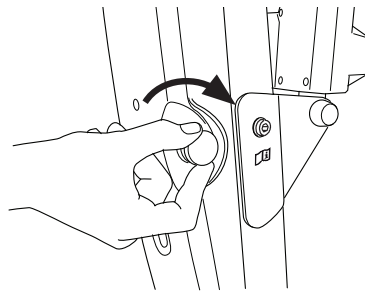

8. Reset the emergency stop by turning the button in the direction indicated by the arrows.


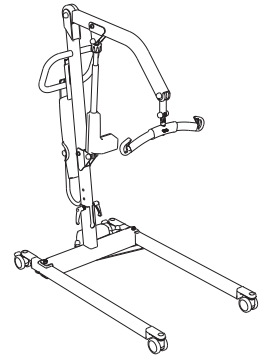


9. Before using the lift for the first time, charge the battery for a minimum of 12 hours, see page 10.

After assembly, check to ensure that:

- lift arm motions correspond with the buttons on the hand control
- emergency lowering (mechanical and electrical) functions properly
- wheel brakes work properly
- base-width adjustment works properly
- the lift is charging.

Operation

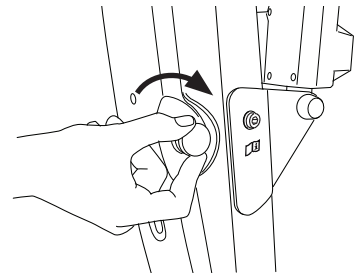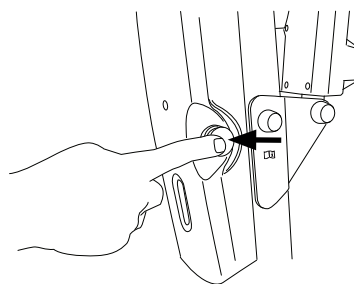

Hand control

Operate the lift using the pushbuttons on the handcontrol. For raising and lowering, press either of the two upper push-buttons. Directional arrows show the direction of movement (up/down) when the hand control is held as illustrated. For base-width adjustment, press either of the two lower push-buttons: wider, narrower. The movement stops when you release the buttons.


Emergency stop

Activate emergency stop:

Push the red emergency stop button on the control unit.


Reset emergency stop:

Turn the button in the direction of the arrows.

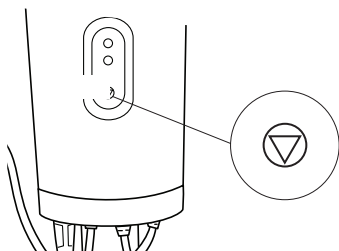


Electrical emergency lowering

The lift arm is lowered electrically by pressing the "⏏" -button".

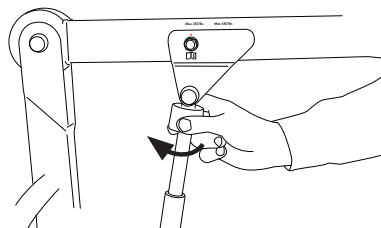


Mechanical emergency lowering

The lift arm is lowered mechanically by turning the red emergency-lowering cylinder in the direction of the arrows (clockwise).

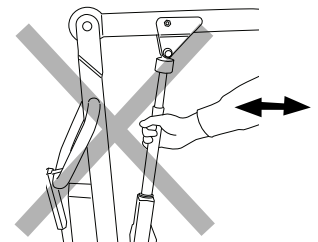


⚠ Never move the lift by pulling the actuator!

Locking

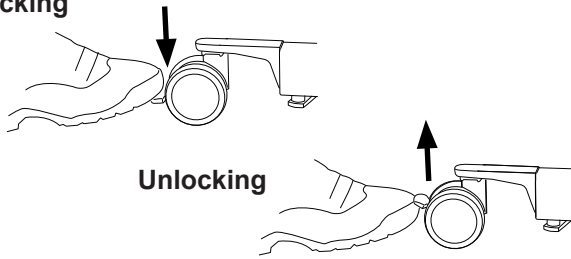

Unlocking



Locking the wheels

The rear wheels can be locked for rotation and lateral movement. To lock the wheels press the brake pedal down with your foot. Release the wheels by pressing the pedal up.

During lifting, wheels should remain unlocked so that the lift may shift to the patient's center of gravity. The wheels should however be locked if there is a risk for the lift moving into the patient, for example when lifting from the floor.

△ Locked wheels during lifting increases the risk of the lift tilting over.

Quick reference guide

A quick reference guide comes with the lift and should be kept easily accessible in its holder on the lift mast, so that users of the lift may easily remind themselves about the use of the lift.

△ NOTE! The quick reference guide does not replace the lift's instruction guide.

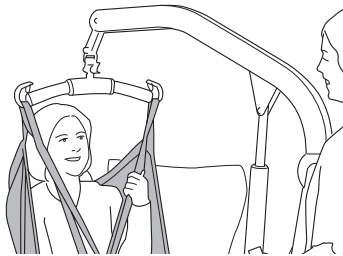



Bild 1.




Bild 2.

Installation of Latches

After installation, ensure that the spring loaded clip is taut against the sling bar and moves freely in the sling bar hook.

Lift correctly!

Before each lift, make sure that:



- the Sling loops at opposite sides of the Sling are at the same height
- all the Sling loops are fastened securely in to the Sling bar hooks
- the Sling bar is level during the lift, see Figure 1.

△ If Sling bar is not level (see Figure 2), lower the user to a firm surface and adjust according to the Sling in use Instruction Guide.



△ An improper lift can be uncomfortable for the user and cause damage to the lift equipment! (see Figure 2).

Position of the Lift when Lifting

From/To: Bed

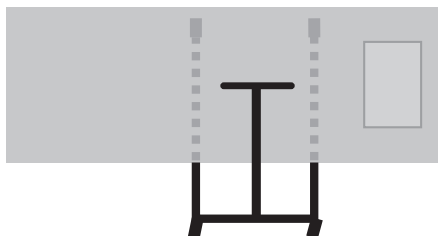



Chair/Hygiene chair



Floor


NOTE: Place a pillow under the patient's head for increased performance and comfort. Always have the wheels locked when lifting from the floor.

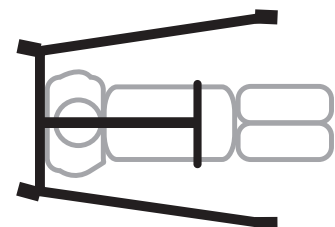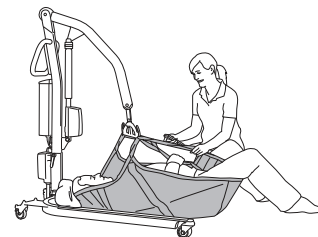

Adjustments

Adjustment of maximum load

For guidance on adjustment alternatives, see "Adjustments of maximum load/lifting height", page 5.

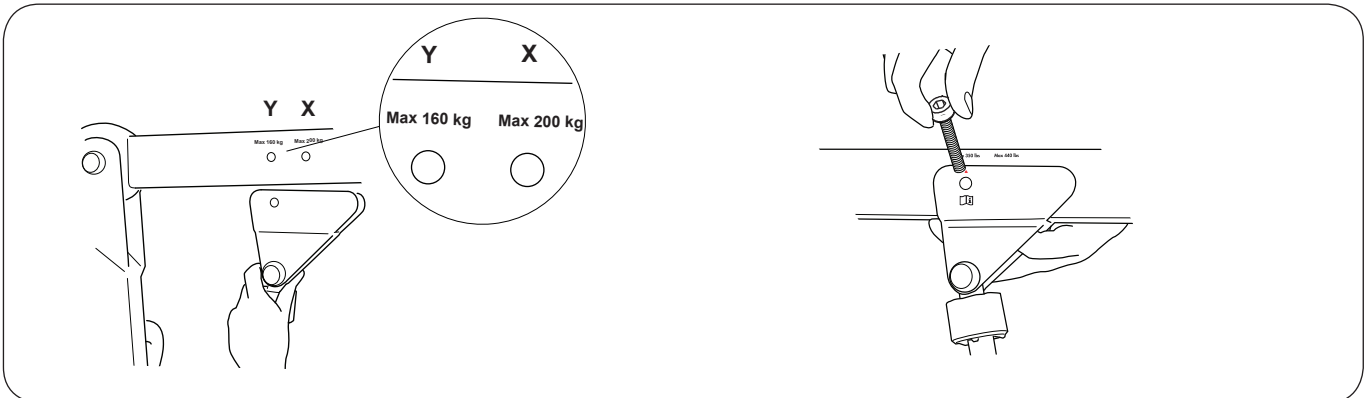


1. Use Allen wrench 8 mm and closed-end wrench 17 mm to dismount the upper lift motor attachment from lift arm. For maximum load 160 kg/350 lbs choose position (Y) on the lift arm. For maximum load 200 kg/440 lbs choose position (X) on the lift arm.

Note! Study the markings on the lift.

On delivery, the lift is set for a max. load of 160 kg/350 lbs), in position (Y).

2. Secure the upper lift motor attachment in desired position using accompanying bolt and locking nut. Use Allen wrench 8 mm and closed-end wrench 17 mm.

Adjustment of lifting height

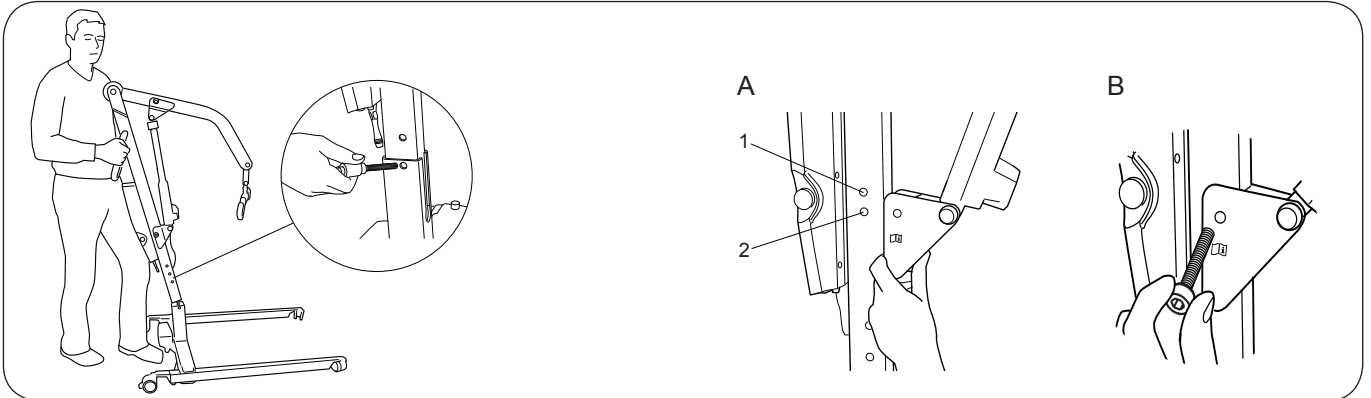

Via the lift mast

Release the lift mast by loosening the locking handles. The lifting height can be adjusted in three different levels on the lift mast. Choose one of the three holes according to the illustration above. The middle hole is recommended in most cases. The lower hole is recommended when extra lifting height is needed. The upper hole is recommended when a lower lifting height is needed. Secure the lift mast by using the accompanying locking handles. Adjust the position of the handles so that they point downward.

The distance between two holes is 50 mm.

See "Table of measurements", page 5.


If this adjustment not is sufficient, see "Adjustment of lifting height - Via the lower lift motor attachment", page. 9.

Via the lower lift motor attachment

- A. Use Allen wrench 8 mm and closed-end wrench 17 mm to dismount the lower lift motor attachment from the lift arm. Choose the upper hole (1) for a higher lifting height and the lower hole (2) for a lower lifting height.
- B. Secure the lower lift motor attachment in desired position using accompanying bolt and locking nut. Use Allen wrench 8 mm and closed-end wrench 17 mm.

On delivery, the lower lift motor attachment is mounted in the lower hole (2).

Charging the Batteries

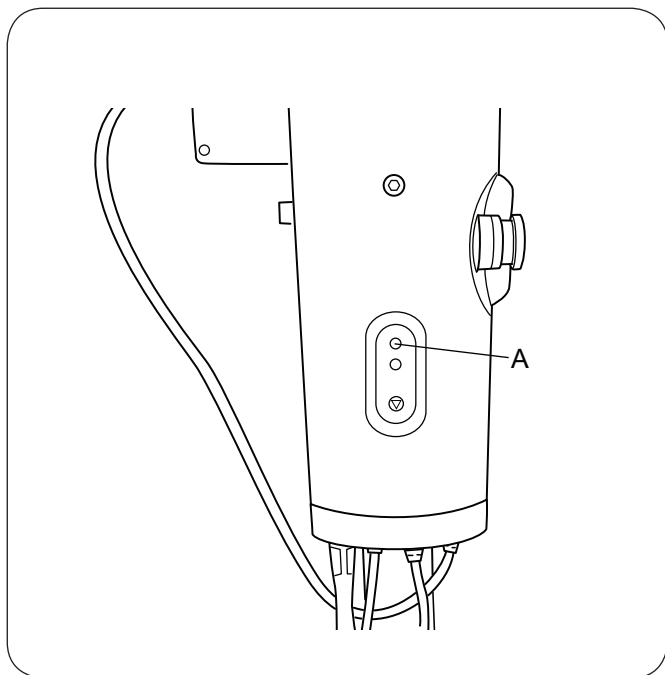

For maximum battery life, batteries must be charged regularly. We recommend charging after use or each night. If the lift is not in daily use, we recommend that the emergency stop be pressed in after the lift has been used. This breaks the current and conserves battery power. Make sure the lift is fully charged before pressing in the emergency stop.


On the control unit there is a display with a yellow LED (A) that illuminates while the charger is connected to an electric socket. Maximum charge is reached after about 12 hours. When the batteries are fully charged, the charger switches automatically to maintenance charging.

When battery capacity is low (approx. 2-10 lift cycles remain) an audible signal sounds. In this case, charge the lift immediately.

Never charge batteries in a wet area!

The lift cannot be charged with the emergency stop button activated.

Charging procedure

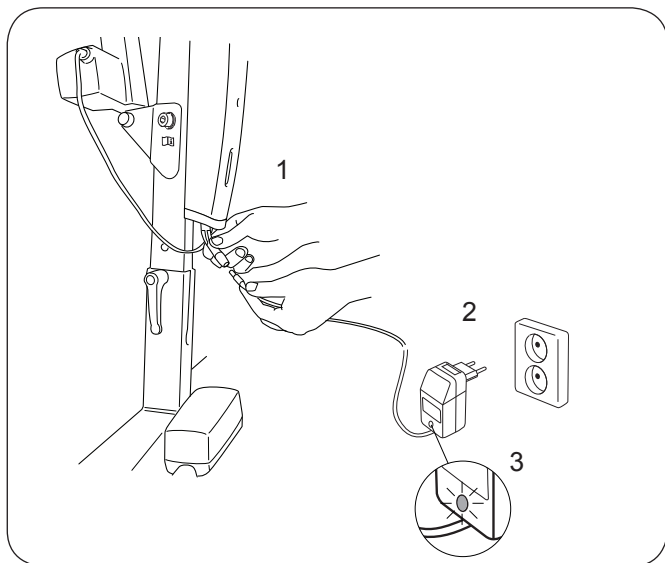

With external charger:

1. Connect the charger cable to the charger socket under the control unit.
2. Connect the charger to a 100-240 V AC electric socket.
3. When the charger is connected a LED indicates:
 - yellow light indicates charging
 - green light indicates maintenance charging.

Note! The lift does not operate when the charger cable is plugged into an electric socket.



Old batteries are to be left at the nearest recycling station or given to personnel authorized by Liko/Hill-Rom.

Maximum Load

Different maximum allowable loads may apply to different products on the assembled lift system: lift, sling bar, sling and other accessories. For the total lift system, the lowest max. allowable load indicated for the respective products on the system always applies. For example: An Uno 200 that is approved for 160 kg (350 lbs)/200 kg (440 lbs) may be equipped with a lifting accessory that is approved for 300 kg (660 lbs). In this case, the applicable max. load is 160 kg(350 lbs)/200 kg (440 lbs) for the total lift system.

Study markings on the lift and lifting accessories or contact your Liko/Hill-Rom representative if you have any questions.

Recommended Lifting Accessories

△ Use of accessories other than those recommended may entail risk.

Sling bars and accessories recommended for use with Uno 200 are described below.


Changing sling bars and adding extra accessories affects the maximum lifting height of the lift. Before changing sling bars and accessories, it is important to ensure that it will still be possible to achieve the desired lifting height for situations in which the lift will be used.

For choice of appropriate slings and other accessories, consult our brochure "Lifting Accessories". For further guidance when selecting slings, study the instruction guides for the respective sling models. Here, you will find advice on suitable combinations of Liko sling bars and Liko slings.

Contact your Liko/Hill-Rom representative or visit www.liko.com for advice and information on Liko's range.


SlingBar Mini 220
Max 205 kg / 450 lbs.

Prod. No. 3156005




Universal SlingBar 350
Max 300 kg / 660 lbs.

Prod. No. 3156074




Universal SlingBar 450
(Standard for Uno 200)
Max 300 kg / 660 lbs.

Prod. No. 3156075




Universal SlingBar 600
Max 300 kg / 660 lbs.

Prod. No. 3156076




Universal TwinBar 670
Max 300 kg / 660 lbs.

Prod. No. 3156077




Sling SideBars 450
incl. storage bag
Max 300 kg / 660 lbs.

Prod. No. 3156079




Sling Cross-bar 450
Max 300 kg / 660 lbs.

Prod. No. 3156021



Sling Cross-bar 670
Max 300 kg / 660 lbs.

Prod. No. 3156018



SlingBar Cover Paddy 30


Prod. No. 3607001

(fits Universal SlingBar 350, 450 and 600
and SlingBar Slim 350)



Bag for SlingBars

Prod. No. 2001025




Quick-release Hook

Liko's Quick-release Hook system enables quick and easy exchange of lifting accessories on Liko's mobile and stationary lifts. Uno 200 requires Q-link 13 for use with Quick-release Hook.


Quick-release Hook Universal fits Universal SlingBar 350, 450 and 600 (Prod. No. 3156074-3156076). Quick-release Hook TDM fits SlingBar Mini 220 (Prod. No. 3156005), Sling Cross-bar 450 and 670 (Prod. No. 3156021 and 3156018) and Universal TwinBar 670 (Prod. No. 3156077).

When a sling bar mounted with the Quick-release Hook system is used, the lifting height will be 33 mm shorter than with a permanently mounted sling bar.

See "Guide to Liko's Quick-release Hook System", which can be downloaded from our website, www.liko.com, or contact Liko/Hill-Rom for more information on the advantages and use of the Quick-release Hook system.



**Quick-release Hook
Universal**
Prod. No. 3156508



**Quick-release Hook
TDM**
Prod. No. 3156502




Q-link 13
Prod. No. 3156509

Scale

In need of weighing persons in combination with Uno 200 we recommend LikoScale 350 (Adapter 12 mm is required).
Max. load 350 kg (770 lbs).

LikoScale 350 is certified according to the european directive NAWI 90/384 (Non Automatic Weighing Instruments).

Contact Liko/Hill-Rom for more information.



LikoScale 350
Prod. No. 3156228



Adapter 12 mm
Prod. No. 2016504

Simple Troubleshooting

**The lift does not work up/down.
Width adjustment does not work
in/out.**



1. Check that the emergency stop button is not pushed in (p. 7).
2. Check that the cables to the control unit are correctly connected (p. 6).
3. Check that the charger cable is not connected to an electric socket.
4. Check that the battery is charged (p. 10).
5. *If the lift still does not work satisfactorily, contact Liko-Hill-Rom.*

Battery charging does not work.



1. Check that the emergency stop button is not pushed in (p. 7).
2. Check to ensure that the electric socket is power-supplied.
3. Check that the charger cable is correctly connected (p.10).
4. *If the lift still does not work satisfactorily, contact Liko/Hill-Rom.*

The lift stops in the elevated position.



1. Check that the emergency stop button is not pushed in (p. 7).
2. Use the electrical emergency lowering to lower the patient to a stable underlying surface (p 8).
3. Use the mechanical emergency lowering to lower the patient to a stable underlying surface (page 8).
4. Check that the battery is charged (p.10).
5. *If the lift still does not work satisfactorily, contact Liko/Hill-Rom.*

If you hear unusual sounds.



Contact Liko/Hill-Rom.

Care and Maintenance

Care and inspection

To ensure trouble-free operation, certain components should be checked each day the lift is used:

- Inspect the lift and check for any signs of external damage.
- Check the fixture of the sling bar.
- Check safety latch function.
- Check raising, lowering and base-width adjustment.
- Check the emergency lowering function (both electrical and mechanical).
- Charge the batteries each day the lift is used and check charger function.

When necessary, clean the lift with a moist cloth and check that the wheels are free from dirt. Find more detailed information regarding cleaning and disinfection of your Liko/Hill-Rom product in the document Care and Maintenance at our website: www.liko.com.

△ The lift should not be exposed to running water.

Service

Uno 200 must be inspected at least once per year, with particular attention to parts that are subject to wear.

△ Repairs and maintenance may only be carried out in accordance with Liko/Hill-Rom service manuals, by authorized Liko/Hill-Rom service personnel and using original Liko/Hill-Rom spare parts.

Service agreements

Liko/Hill-Rom invites you to sign a service agreement for regular maintenance and inspection of your Liko/Hill-Rom product.

Transportation and storage

During transportation, or when the patient lift is not to be used for some time, the emergency stop button should be pushed in. The environment where the patient lift is transported and stored should have a temperature between 10 °C and 40 °C and a humidity between 30 % and 75 %. The air pressure should be between 700 and 1060 hPa.

Recycling

For instructions on how your Liko/Hill-Rom product should be recycled, please visit our website: www.liko.com.

Product changes

Liko's products undergo continuous development, which is why we reserve the right to make product changes without prior notice. Contact your Liko/Hill-Rom representative for advice and information about product upgrades.

Design and Quality by Liko in Sweden

Hill-Rom's Management system are certified in accordance with ISO 9001 and its equivalent for the medical device industry, ISO 13485. Hill-Rom's Management system is also certified in accordance with environmental standard ISO 14001.



A  Company

www.liko.com

Manufacturer:

Liko AB
Nedre vägen 100
SE-975 92 Luleå
Sweden
info@liko.se